



COMPRESSOR NEBULIZER Guidebook



**Please read this guidebook
carefully before operating this unit.**

Your Nebulizer is intended for use in the treatment of asthma, COPD and other respiratory ailments in which an aerosolized medication is required during therapy. Please consult with your physician and/or pharmacist to determine if your prescription medication is approved for use with this Nebulizer. This Nebulizer is intended for single patient use.



COMPRESSOR NEBULIZER Efficient Respiratory Therapy

INSTRUCTIONS

Contents

1. INTRODUCTION	2
2. PRODUCT IDENTIFICATION	3
3. IMPORTANT SAFEGUARDS	4
4. OPERATING YOUR COMPRESSOR NEBULIZER.....	5
5. CLEANING.....	6
6. SPECIFICATIONS	7

1. INTRODUCTION


Thank you for purchasing the Easy Neb Compressor Nebulizer. It is a compact medical device designed to efficiently deliver physician prescribed medication to the bronchial lung passages. With proper care and use, it will provide you with many years of reliable treatment.

This product is developed for successful treatment of asthma, allergies and other respiratory disorders. It creates a stream of air that travels through a clear tube to the nebulizer. When air enters the nebulizer, it will convert the prescribed medication into an aerosol mist for easy inhalation.

Your Easy Neb Compressor Nebulizer should be used in accordance with the directive given to you by a licensed physician and/or a respiratory therapist. We encourage you to thoroughly read this guidebook to learn about the features of this product. Any use of this product other than its intended use should always be avoided.

Your product is covered under a limited 2 Year warranty. Register your product immediately after purchase at www.homeaide.us/warranty.html

2. PRODUCT IDENTIFICATION

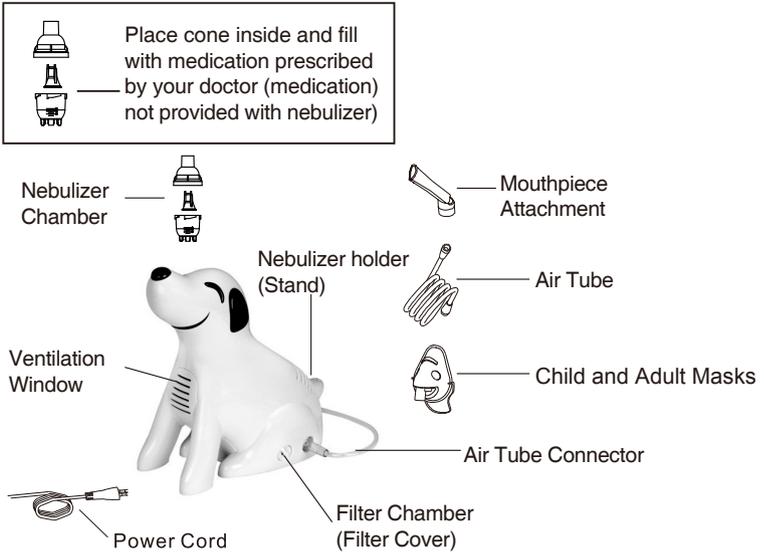

Note: Note: Read all instructions carefully before use.

The following lists the basic precautions needed when using an electrical product:

Caution: Failure to read and observe all precautions could result in personal injury or equipment damage.

3. IMPORTANT SAFEGUARDS

Product cautions:

1. To avoid electrical shock: Keep the unit away from water
 - a. Do not immerse the power cord or the unit in liquid
 - b. Do not use while bathing
 - c. Do not reach for a unit that has fallen into water
2. Never operate the unit if it has any damaged parts (including power cord) or if it has been dropped or submerged in water.
3. The unit should not be used where flammable gas, oxygen or aerosol spray products are being used.
4. Disconnect the unit from the electrical outlet before cleaning, filling and after each use.
5. Use of attachments not provided with this nebulizer voids all product warranty.

Operating Cautions:

1. Connect Nebulizer to an appropriate voltage outlet (120V, 60Hz power) (1.3A current).
2. Do not leave this product unattended while running.
3. Never operate the unit if it has a damaged cord or plug, if it has been dropped, or in any way submerged into water, or if it does not work properly.
4. If any abnormality occurs, discontinue use immediately and call 1-800-915-0116.
5. Always unplug the product after every use.
6. Never block the ventilation window of the main unit or place it where the openings may be obstructed.

Storage Cautions:

1. Do not store the unit under direct sunlight, high temperature or humidity.
2. Keep the unit out of reach of small children.
3. Always keep the unit unplugged while not in use.

Cleaning Cautions:

1. Do not immerse the unit in water. It may damage the unit.
2. Disconnect the unit from the electrical outlet before cleaning.
3. Clean all necessary parts after each use as instructed in this guidebook

4. OPERATING YOUR COMPRESSOR NEBULIZER

Note: Prior to initial operation, the nebulizer should be thoroughly cleaned.

1. Place your Compressor Nebulizer on a flat and stable surface.
Be sure that you can easily reach the controls when you are seated.
2. Gently twist the top part of the nebulizer cup counter-clockwise to disassemble.
3. Fill the bottom section of the nebulizer cup with the medication prescribed by your physician. Be sure that the cone is placed inside the bottom section.



4. Gently twist the top part clockwise to reassemble the nebulizer cup. Be sure the two sections fit well.
5. Attach one end of air tube to the base of the nebulizer chamber.
6. Attach the other end of air tube to the tube connector located on the side of the compressor.
7. Attach mouthpiece or mask to the top section of the nebulizer.
8. Plug the power cord into an appropriate electrical outlet.
(Make sure at this stage, the power switch is at "OFF" status.)
9. Press power switch to begin your prescribed treatment.

IMPORTANT:

The compressor motor has a thermal protector which will shut off the unit before the unit overheats. When the thermal protector shuts the unit off, please:

- a. Double check the unit is off.
 - b. Unplug the unit from the electrical outlet.
 - c. Wait 30 minutes for the motor to cool down before attempting another treatment. Make sure the ventilation window is not obstructed.
10. When treatment is finished, shut off the unit and unplug it from the electrical outlet.

5. CLEANING

Cleaning & Disinfection for the Nebulizer's Accessories (including: nebulizer cup, mouthpiece, Air filters (5pcs), child mask, adult mask, air tubing)

Care guidelines for Nebulizer Accessories after each use

1. Clean the Nebulizer's Accessories with the distilled water
2. Completely immersed the Nebulizer's Accessories (not the nebulizer unit) into approximately 75% isopropyl alcohol
3. Soak accessories for approximately 30 minutes
4. Wash and rinse the Nebulizer's Accessories with about 50°C (122°F) water.
5. Shake out water, then dry with a clean, soft cloth or leave to air-dry in a clean place.
6. Make sure that the Nebulizer's Accessories and other cleaned parts are completely dry then put all these parts in a dry sealed container.

Nebulizer Filter Care

1. Do not operate without a filter.
2. Only use filters meant for the Easy Neb Nebulizer.
3. Change the filter every 30 days or when the filter turns gray (whichever happens first).
4. Do not use cotton or any other materials to replace filters.
5. Do not wash or clean the filter after use.

Filter replacement procedure:

1. Remove the filter cover
2. Remove used filter
3. Replace with a new filter
4. Replace the filter cover

6. SPECIFICATIONS

Power	AC 120V 60Hz
Power Consumption	1.3A
Nebulizer medication Capacity	6ml
Size Approx.	(78.25±13.08)% within 0.5 to 5um range
MMAD	2.52±0.89um
Average Nebulization Rate	≥0.2ml/min
Noise Level Below	65dBA (DIN EN 13544-1, at 1 meter)
Compressor Pressure Range	30 ~ 50 Psi / 206Kpa~345Kpa
Operation Pressure Range	9.5 ~ 16 Psi / 65.5Kpa~110Kpa
Liter Flow Range	6~10 lpm
Operation Temperature Range	10°C ~to 40°C (50°F ~104°F)
Operation Humidity Range	10% ~95% RH
Storage Temperature Range	-20°C~to 70°C (-4°F~158°F)
Storage Humidity Range	10%~95% RH
Atmospheric pressure	500~1060hPa
Dimension (LxWxH)	120x200x215mm
Weight	1.4kg
SH-B type Standard accessories available	Nebulizer bottle(6ml), Air tube(1.6m), Mouthpiece, Adult mask, Child Mask, Air filters (5pcs)

Protection against electric shock:

- Class II Equipment
- Type BF applied parts: Nebulizer bottle(6ml), Air tube(1.6m), Mouth piece, Adult mask, Child Mask, Air filters (5pcs)



Manufactured for:
Home Aide Diagnostics, Inc.
1072 S. Powerline Rd.
Deerfield Beach, FL. 33442
(800) 915 – 0116